


-15kV TOF: -9181 v  
 -3.6kV MCP: -3364 v  
 -2.4kV MCP: -1784 v  
 Input Cur: 310 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Tue Nov 14 10:18:39 2006

## TIDE Direct Events

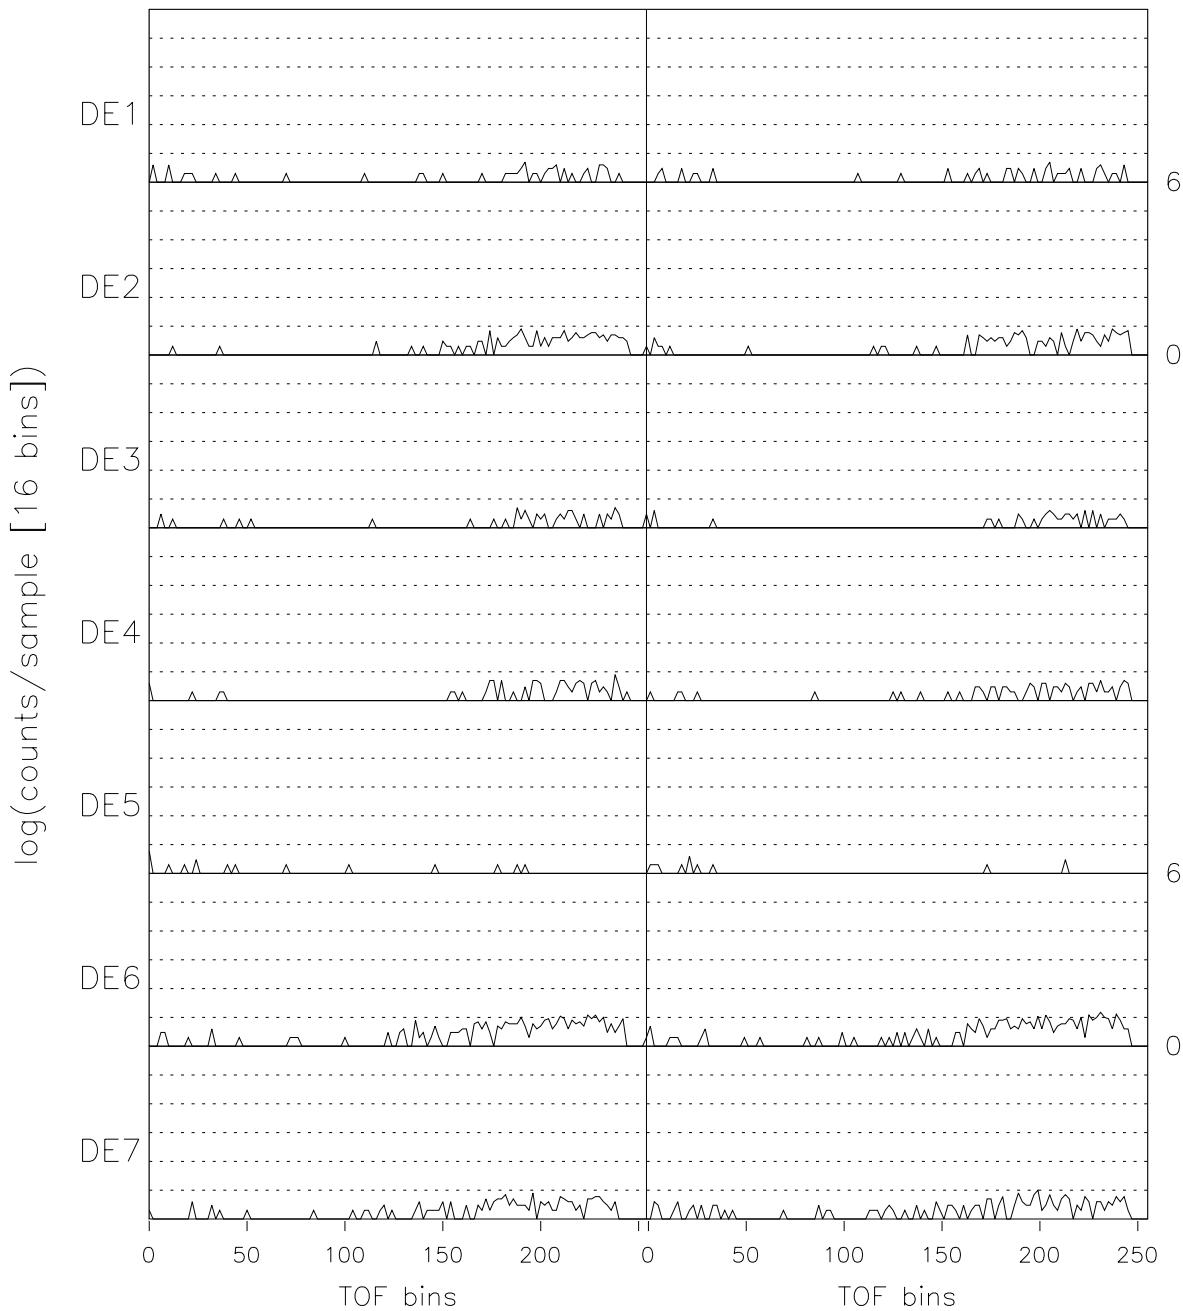

reported: 10-28-06 09:29:51 UT

reported: 10-28-06 09:33:03 UT

file: /export/data/tide/nrt/06102801.dat

-15kV TOF: -9181 v

-3.6kV MCP: -3379 v

-2.4kV MCP: -1784 v

Input Cur: 316 ma

RPA max: 237 v

Mirror max: 238 v